


# **Medicare Nurse Call System Connections**

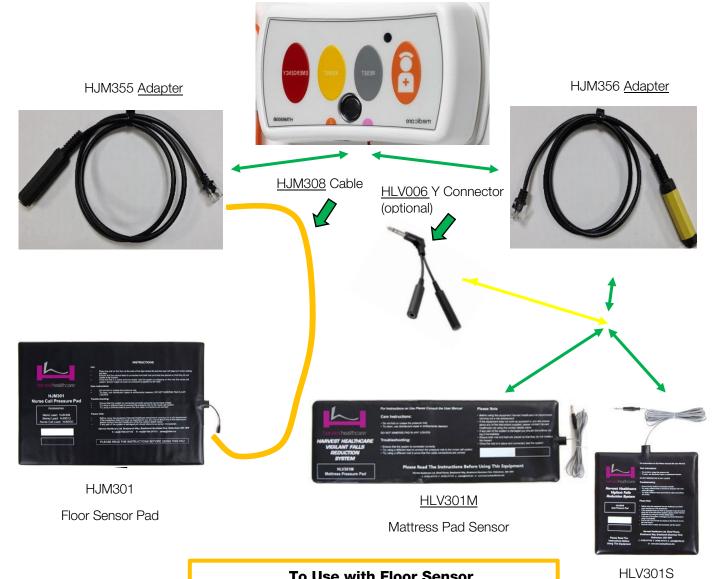

### To Use with Floor Sensor

- 1. Connect a <u>HJM355</u> adapter into the nurse call system.
- 2. Connect one end of a HJM308 cable into the HJM355 and the other end into the HJM301 floor sensor.

#### To Use with Mattress or Seat Sensor

- 1. Connect a <u>HJM355</u> adapter into the nurse call system (note the yellow colour on the plug).
- 2. Plug either the HLV301M or the HLV301S sensor mats into the HJM355 adapter.
- 3. You can use HLV006 Y connector to connect a seat and mattress sensor to the same HJM355 adapter.
- 4. If the chair is located away from the bed, you can use a HLV006E 6-meter extension cable.

Seat Pad Sensor

- Carry out a risk assessment to ensure this system is suitable for intended use and test system for correct operation each time before use.
- If using a seat pad and mattress pad only one can be in use at any time.
- Read the HJR075 alarm system instructions carefully.
- If you have any doubts about the above, please contact Harvest Healthcare Ltd.

# Stereo Jack-Plug

A stereo jack plug can be identified by the 2 black insulation bands.



# Mono Jack-Plug

A mono jack plug can be identified by the single black insulation band.

#### **HJRM355 ADAPTER**

Used to connect he floor mat to the nurse call system



# **HJM356 ADAPTER**

Used to connect the seat or mattress sensors to the system.



# **HJM308 CABLE**

6.35 mono jack-plug with 3.5mm mono jack-plug. Used to connect floor mat to HJM355 adapter.



#### **HJM330.M**

6.35MM mono jack-plug with to nurse call button.



# **HLV006 Y Connector**

6.35mm stereo jack-plug to 2 x 6.35mm sockets.

Used to connect either mat and nurse call button to nurse call system.

Or seat and mattress sensors to nurse call system.

